


Supplemental materials for:

Hudson AJ, Benjamin J, Jardeleza T, et al. Clinical interpretation of peripheral pulse oximeters labeled "not for medical use". *Ann Fam Med*. 2018;16(6):552-554.

Supplemental Table 1. “Sports and Aviation” or “Wellness” pulse oximeters

Distributor/Manufacturer	Model
Drive Medical	Fingertip Pulse Oximeter
Devon Medical Products	PC-60C Fingertip Pulse Oximeter
Contec Medical Systems	CMS 50DL Fingertip Pulse Oximeter
Santa Medical	SM-2400 OLED Fingertip Pulse Oximeter
Nonin Medical	Go2 Achieve Personal Fingertip Pulse Oximeter
Quest Products	3-in-1 Fingertip Pulse Oximeter
ChoiceMMed	MD300C52 Fingertip Pulse Oximeter
Octive Technologies USA	300C Fingertip Pulse Oximeter

Supplemental Figure 1. Modified Bland Altman Analysis comparing 8 NMU-PO to MU-PO.

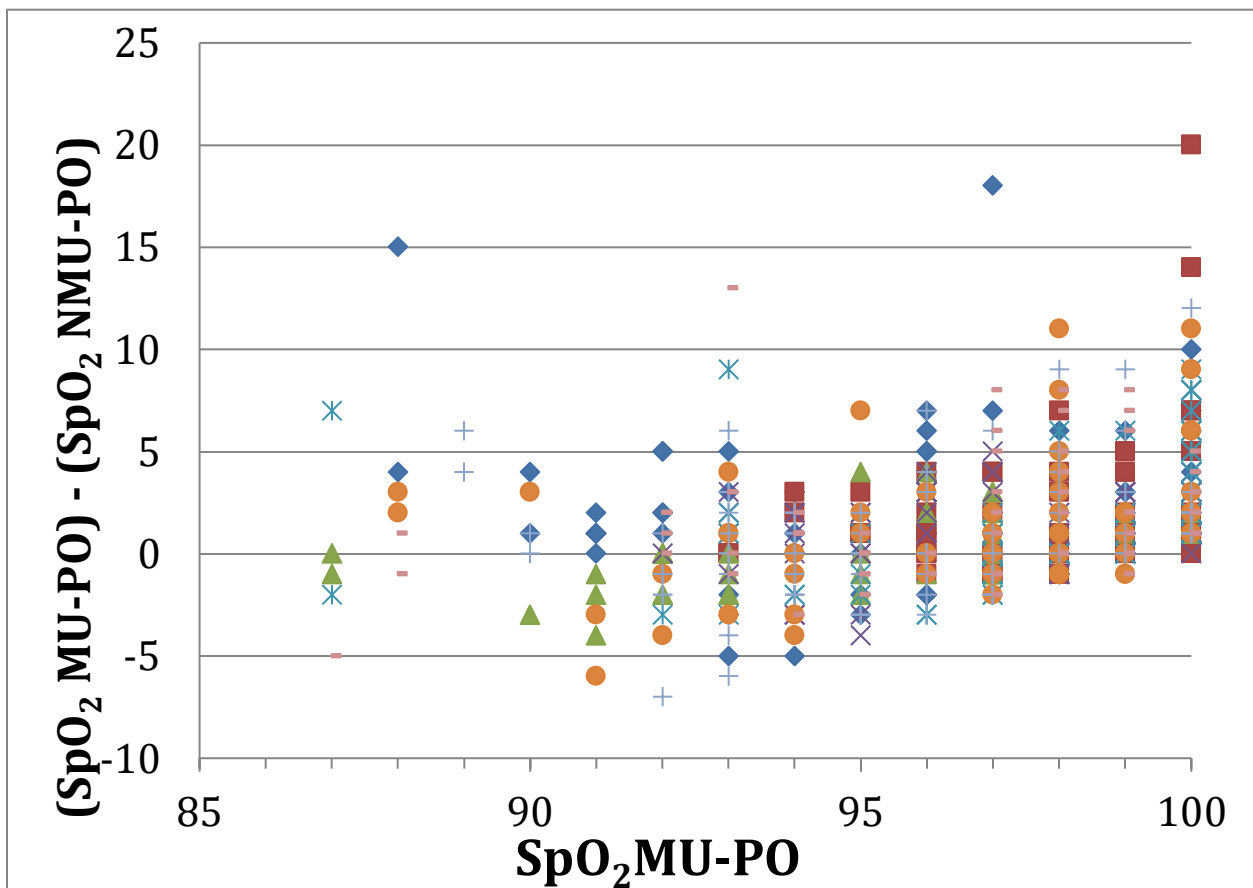

MU-PO = medical use pulse oximeters; NMU-PO = nonmedical use pulse oximeters; SpO₂ = oxygen saturation.